

Kingst[®] AneSure[®] Mini Capnograph and Multigas Monitor

Measurements:

EtCO₂ & Capnogram

Respiration Rate

FiN₂O & Waveform of Nitrous oxide

FiAgents & Waveform of Halothane, Enflurane, Isoflurane, Sevoflurane or Desflurane

Note: Need to manually select one of the above five anesthetic gases.



The Next-generation Point-of-care Capnograph and Multigas Monitor

- Small and super lightweight unit with ultimate portability, ideal for emergency, pre-hospital first aid, patient transit, operating room, ICU
- Large reading display mode clearly visible from more than five meters away.
- Turn on the unit and it is ready to use instantly with no need to calibrate.
- Minimal warm-up time with the first value displayed in 5 seconds, and accurate readings displayed in 15 seconds.
- Advanced automatic atmosphere pressure compensation, and the gas compensation programs to ensure accurate measurement results.
- Data output via USB and connections, compatible with multiple database software systems and Bluetooth printers.
- Sturdy design suitable for use in the challenging clinical environments.

Applied situations:

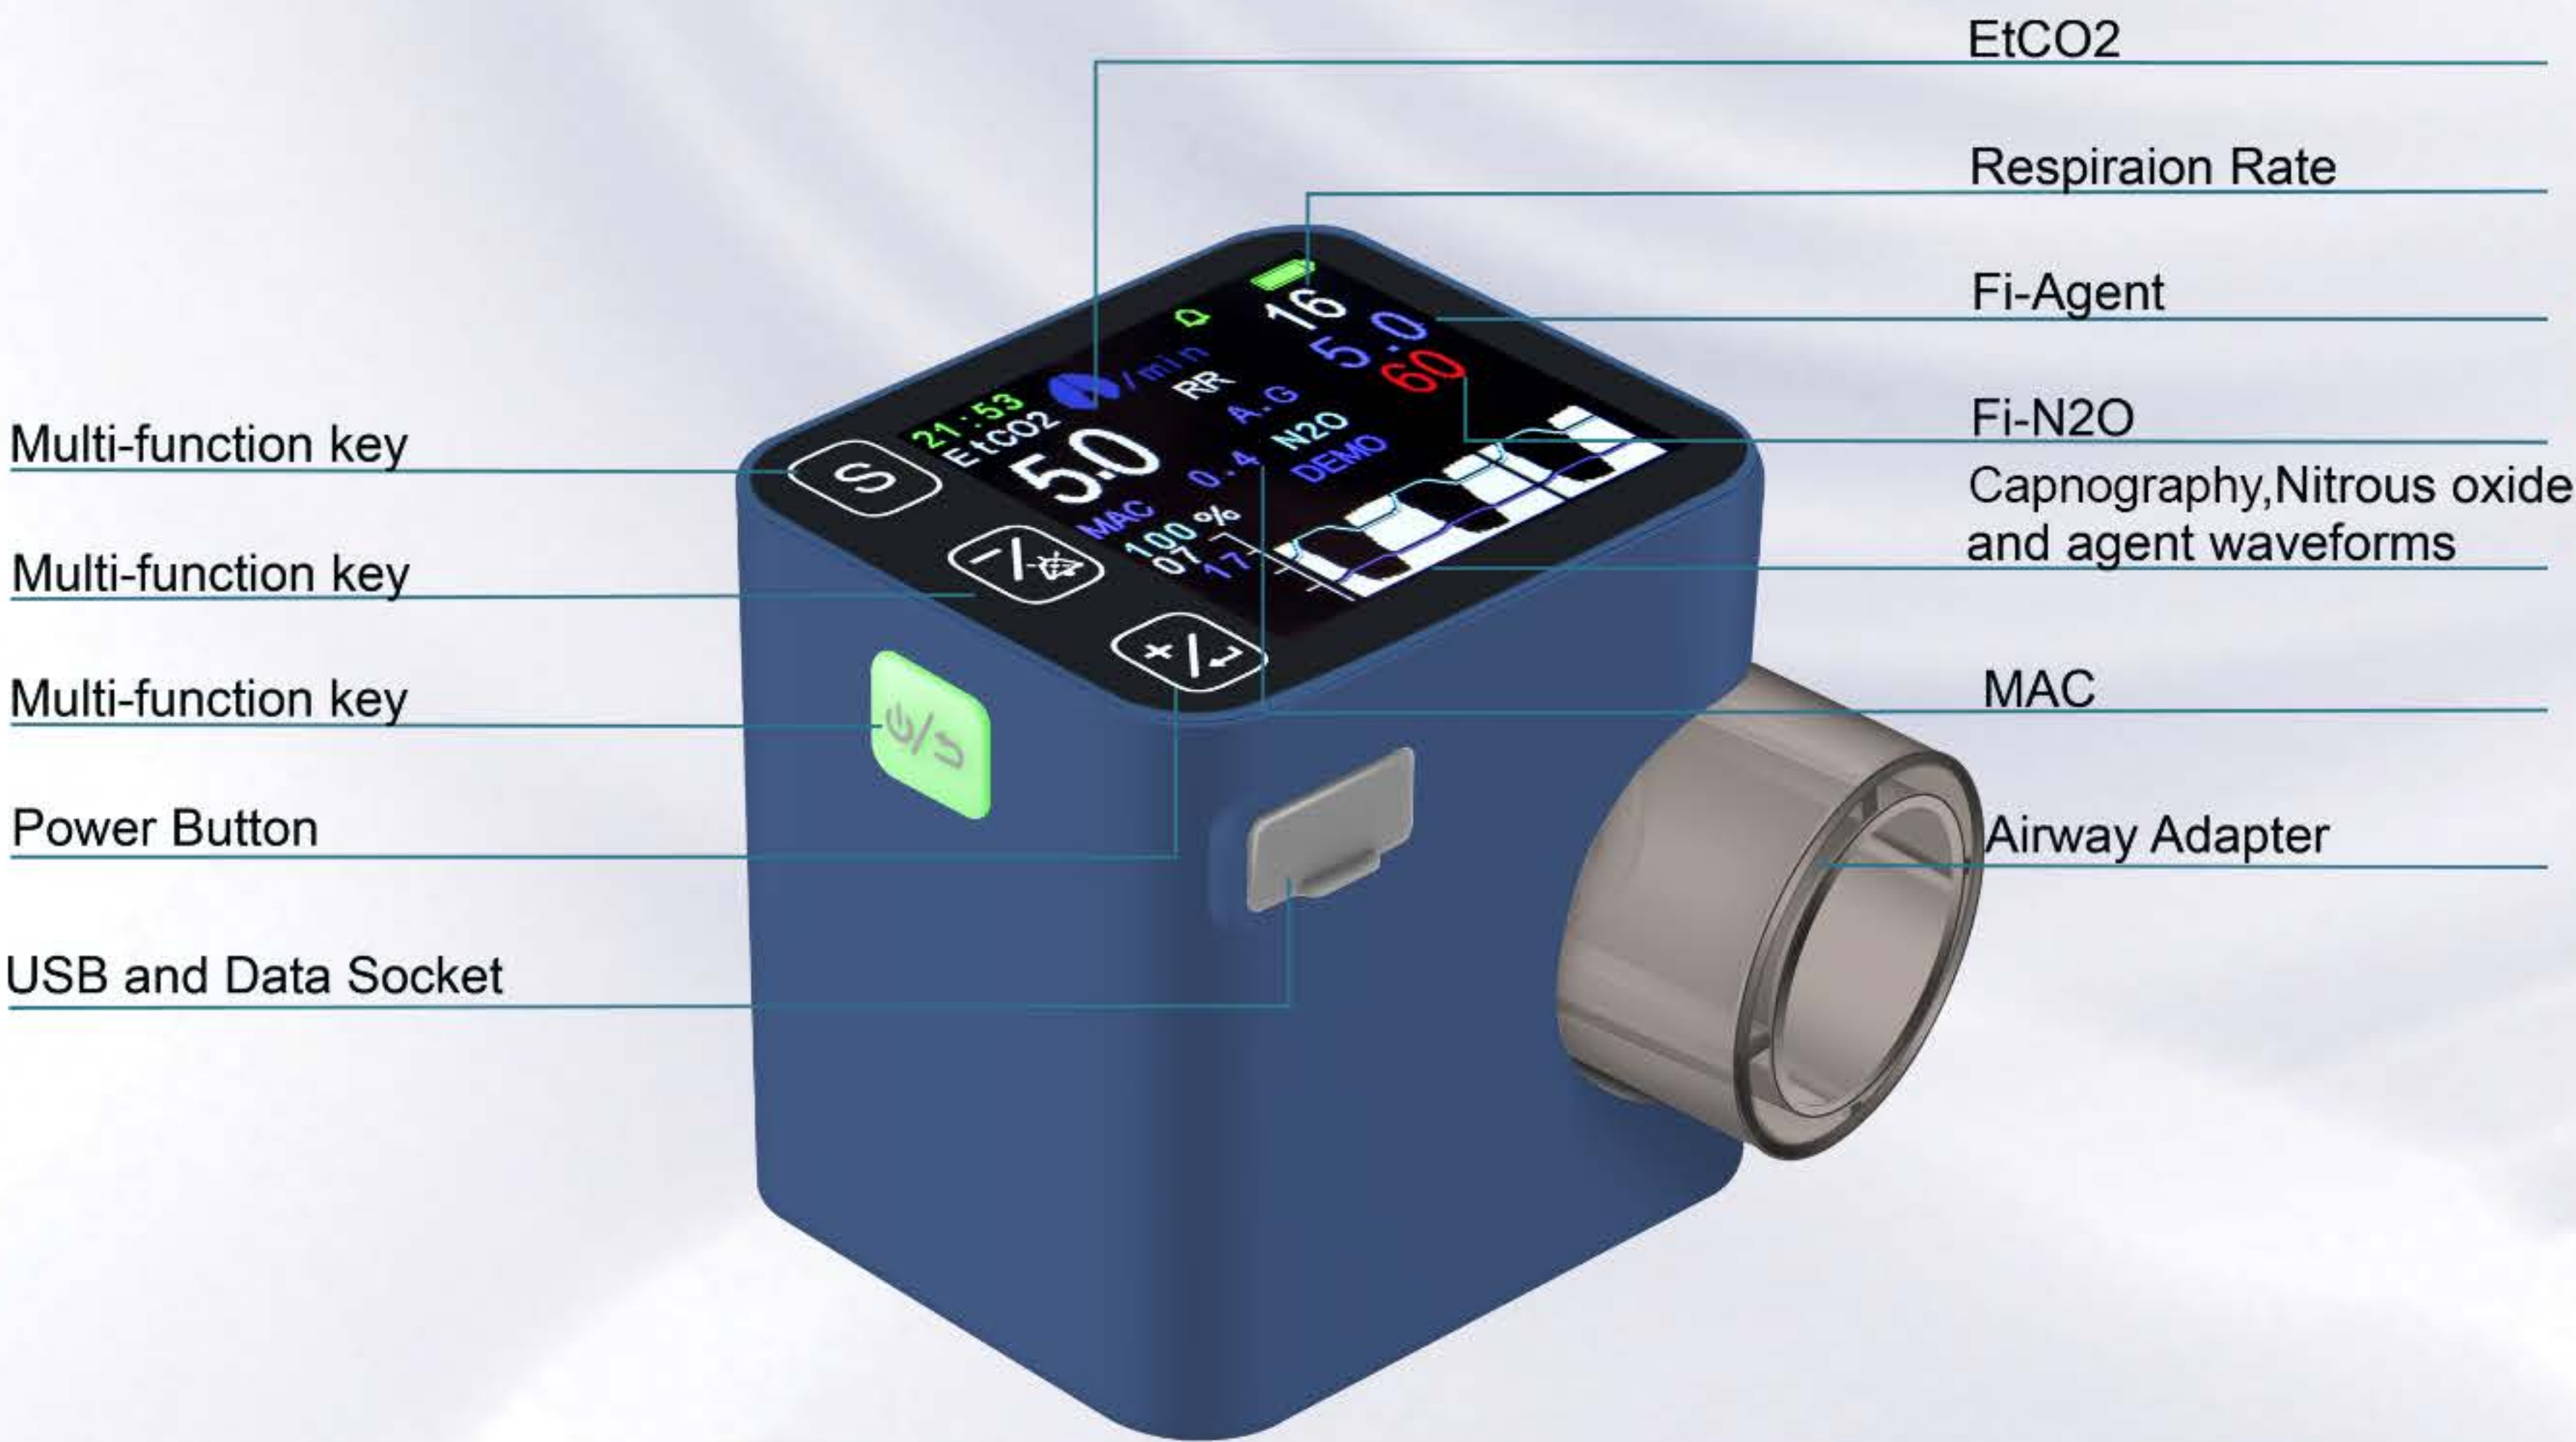
Pre-hospital first aid, hospital transit, emergency department, operating theater, ICU, NICU, etc.

Technical Specifications



Technique: NDIR (Non-dispersive infrared gas analysis)
Power: AC100~240V, 50/60Hz; DC3.7V
Temperature: 5-50℃
Humidity:≤80℃
Atmospheric pressure: 50-120KPa
Battery : Lithium battery, 3.6V,1350mAh, 6 hours (approximately)
Charging time: 4 hours from empty to full
Dimension: 38mm(W)x42mm(H) x44mm(D)
Weight: 80 grams
Display: 1.5”TFT
CO2 Range: 0-19.7%,150mmHg,or 0-20kPa
Accuracy: 0 - 40 mmHg ± 2 mmHg
41 - 70 mmHg ± 5% of reading
71 - 100 mmHg ± 8% of reading
101 - 150 mmHg ± 10% of reading
EtCO2 update: every breath
Trends: 24 hours
N2O Range: 0-100%
Accuracy: ±(2 vol% + 2% of reading)
HAL,ENF,ISO Range: 0-12%
Accuracy: 0-8%: ±(0.15 vol% + 5% of reading)
8-12%: unspecified
SEV Range: 0-15%
Accuracy: 0-10%: ±(0.15 vol% + 5% of reading)
10-15%:unspecified
DES Range: 0-25%
Accuracy: 0-18%: ±(0.15 vol% + 5% of reading)
18-25%: unspecified
All FiAG update: every breath
All FiAG Trends: 24hours
Auto-compensation for atmospheric pressure variation

Respiration rate Range: 3-150 bpm
Accuracy: the bigger value of 1% of reading and ±1bpm
Trends: 24hours
Audible and visual alarm system
Adjustable High and Low EtCO2,RR and FiAG,No Adapter, Clogged Adapter,No Breath (Apnea), Low Battery,so on.
Regulatory: Designed to meet IEC 60601-1:2005+A1:2012(E):Medical electrical equip- ment – Part 1: General requirements for basic safety and essential performance; IEC 60601-1-2:2014: Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral Standard: Electromagnetic disturbances – Requirements and tests; Broad-band random vibration test in accordance with IEC 60068-2-64:2008; Shock test in accordance with IEC 60068-2-27:2008; Free-fall to IEC 60068-2-31:2008
Designed to comply with 93/42/EEC (MDD CE Marking), FDA Standards, Minimum Per- formance and Safety Requirements for Capnometers ISO 80601-2-55-2011: Medical Electrical Equipment performance requirements for the basic safety and essential per- formance of respiratory gas monitors

No futher notification if some technical specification change.Please take update technical specification or test result as the standand



Accessories: Airway Adapter

Airway Adaptor			Patient Type	Color	Weight	Dead Speace	ET tube Size	Materia	Unit Packaging
			Adult/ Pediatric	Brown	7g	5cc	>=4mm	Polycar- bonate	10
			Infant	Brown	11g	1cc	=<4mm	Polycar- bonate	10